


Information 9-1.0.1 I

08.00/01.07

M&C Barometric pressure changing from NN 0 m up to 4.000 m altitude

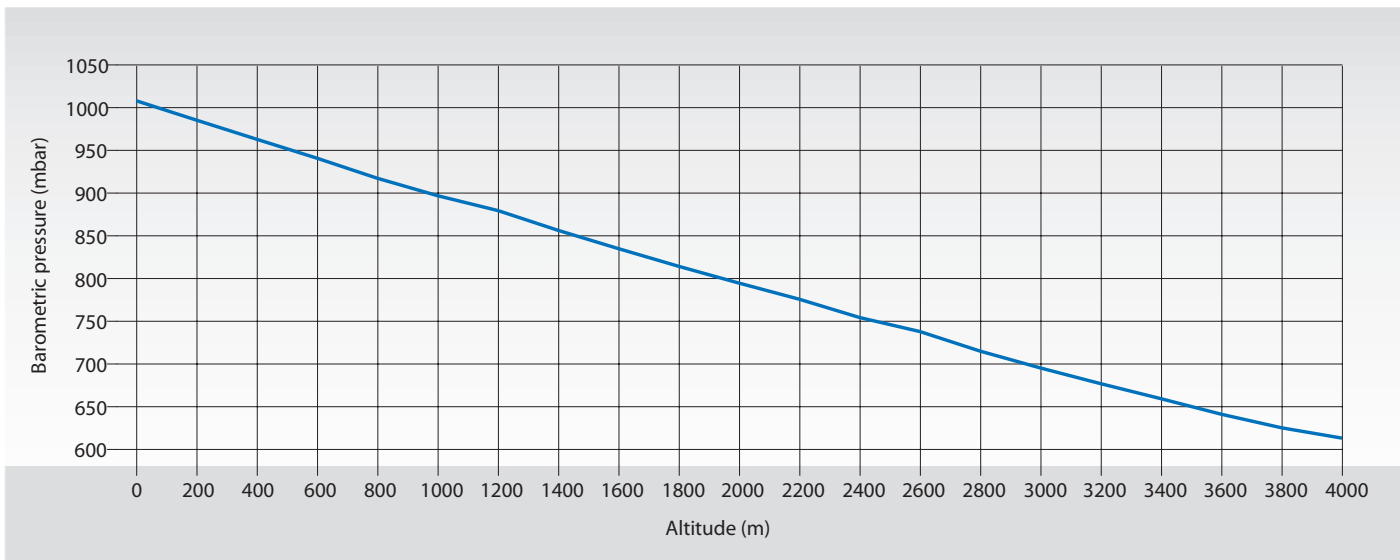

Please check the span calibration when using the oxygen analyzer at different altitudes, normal pressure 1013 mbar = 20,93 Vol.-% O₂.

M&C Span adjustment in (Vol.-% O₂), calibration with air at 1013 mbar

Altitude (m)	O ₂ - Span (Vol.-%)
0	20,93
500	22,20
1000	23,58
2000	26,67
4000	34,42